
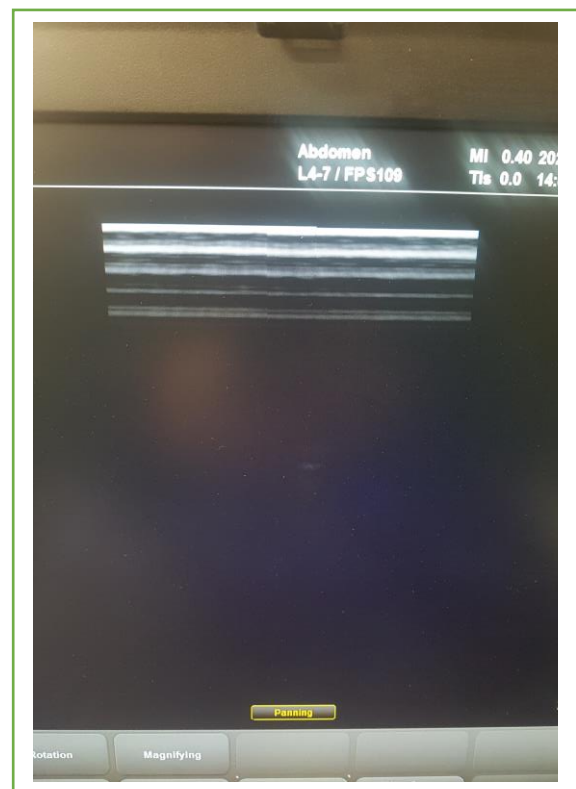


## Ultrasound Transducer Condition Report

<b>Date Tested</b> 1/10/2020	<b>Carried out By</b> – I. Rutherford
<b>Manufacturer</b> – Samsung	<b>Model Number</b> – L4-7
<b>Serial Number</b> – P0R7M3HD900003A	
<b>Transducer Type</b> – Linear	
<b>Date of Manufacture</b> – Unknown	
<b>System used to Test</b> – Samsung HM70A	
<b>Cable</b> – Good	
<b>Lens</b> – Good	
<b>Discolouration</b> –None	
<b>Overall Condition</b> – Good	

© British Medical Auctions

### Airscans –

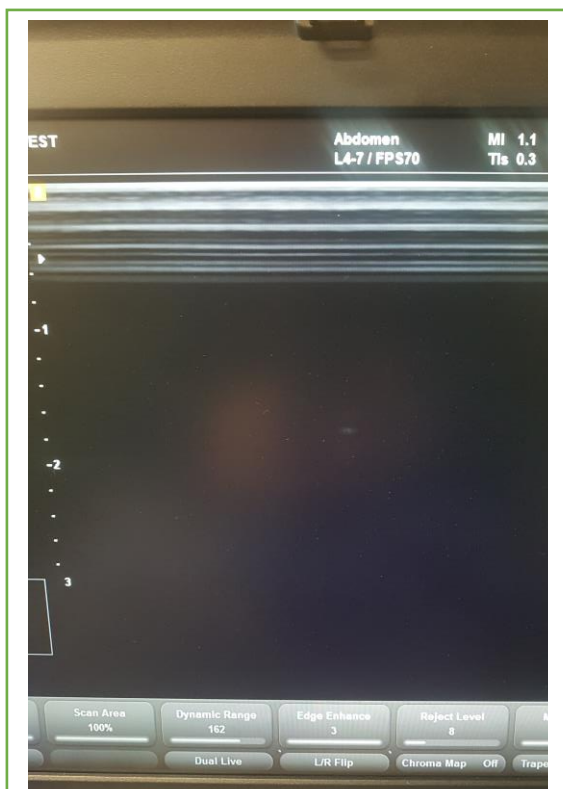

## Ultrasound Transducer Condition Report

<b>Date Tested</b> 1/10/2020	<b>Carried out By</b> – I. Rutherford
<b>Manufacturer</b> – Samsung	<b>Model Number</b> – L5-13
<b>Serial Number</b> – K0JLM3GH500008Z	
<b>Transducer Type</b> – Linear	
<b>Date of Manufacture</b> – 2016-05-10	
<b>System used to Test</b> – Samsung HM70A	
<b>Cable</b> – Good	
<b>Lens</b> – Good	
<b>Discolouration</b> –None	
<b>Overall Condition</b> – Good	

© British Medical Auctions

### Airscans –

