



Ultrasound Transducer Condition Report

Date Tested 2/10/2020	Carried out By – I. Rutherford
Manufacturer – GE	Model Number – M4S-RS
Serial Number – 76876YP2	
Transducer Type – Matrix Array	
Date of Manufacture – July 2011	
System used to Test – GE Vivid S6	
Cable – Good	
Lens – Good	
Discolouration – Minimal	
Overall Condition – Good	

© British Medical Auctions

Airscans –


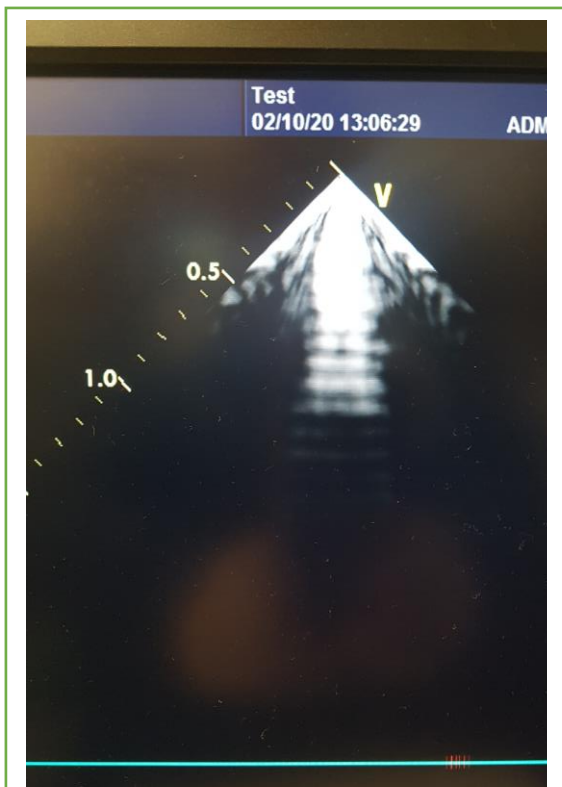


Ultrasound Transducer Condition Report

Date Tested 2/10/2020	Carried out By – I. Rutherford
Manufacturer – GE	Model Number – 12L-RS
Serial Number – 12905YP4	
Transducer Type – Linear	
Date of Manufacture – January 2008	
System used to Test – GE Vivid S6	
Cable – Good	
Lens – Good	
Discolouration – Minimal	
Overall Condition – Good	

© British Medical Auctions

Airscans –

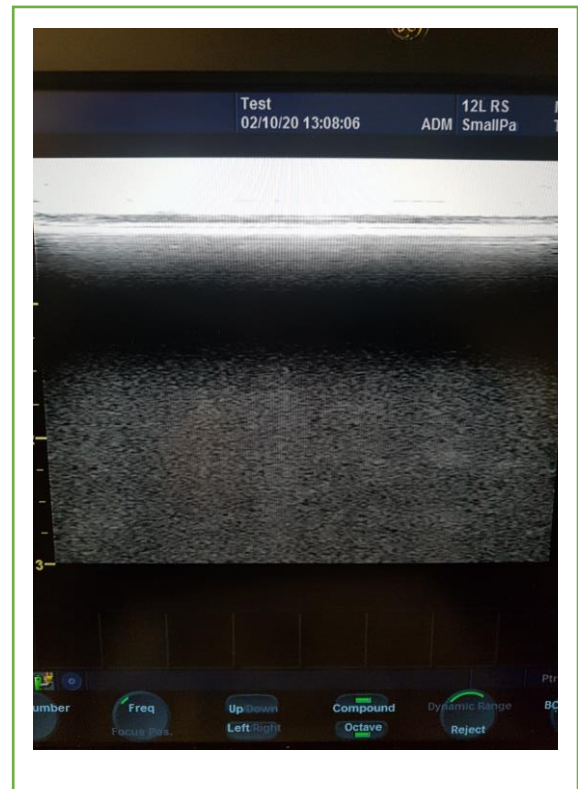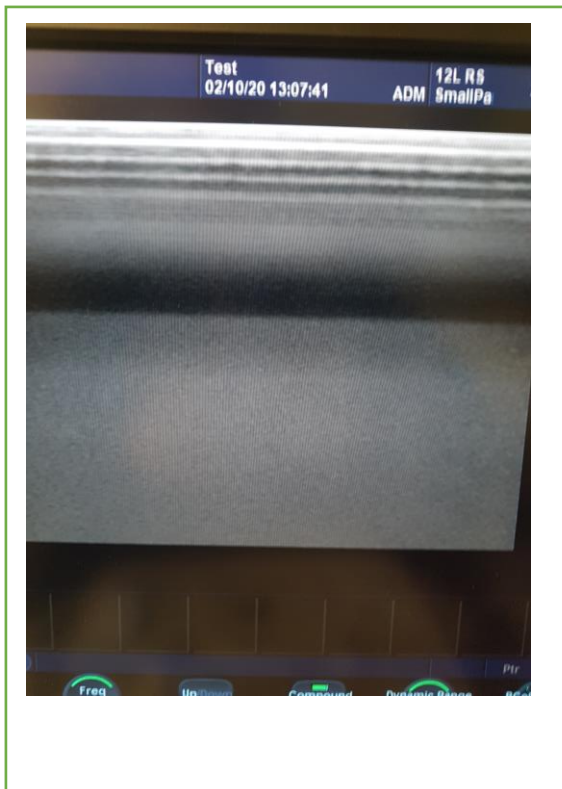

Ultrasound Transducer Condition Report

Date Tested 2/10/2020	Carried out By – I. Rutherford
Manufacturer – GE	Model Number – 10S-RS
Serial Number – 85600PD5	
Transducer Type – Pediatric/Neonatal Sector Array	
Date of Manufacture – March 2008	
System used to Test – GE Vivid S6	
Cable – Good	
Lens – Good	
Discolouration – Minimal	
Overall Condition – Good	

© British Medical Auctions

Airscans –

