
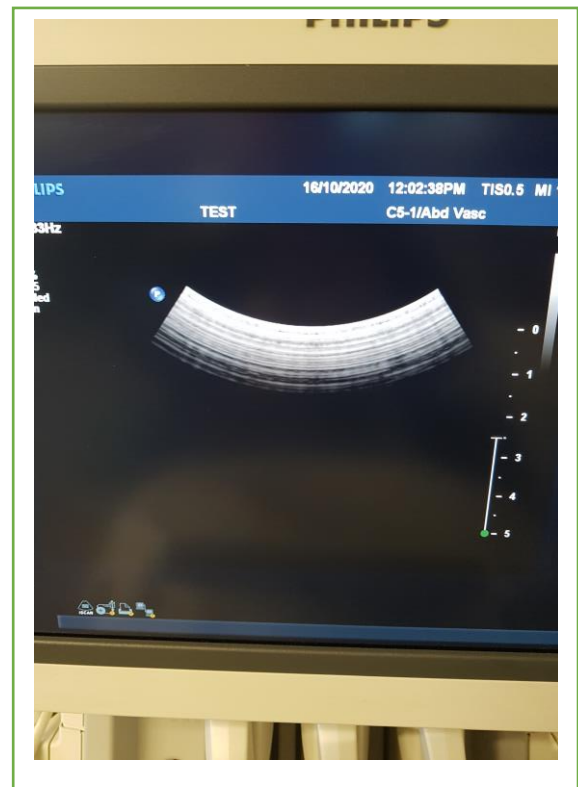


## Ultrasound Transducer Condition Report

<b>Date Tested</b> 16/10/2020	<b>Carried out By</b> – I. Rutherford
<b>Manufacturer</b> - Philips	<b>Model Number</b> C5-1
<b>Serial Number</b> – B03DKR	
<b>Transducer Type</b> – Convex	
<b>Date of Manufacture</b> - Unknown	
<b>System used to Test</b> – Philips iU22	
<b>Cable</b> – Good	
<b>Lens</b> – Good	
<b>Discolouration</b> - Slight	
<b>Overall Condition</b> – Good	© British Medical Auctions

### Airscans –


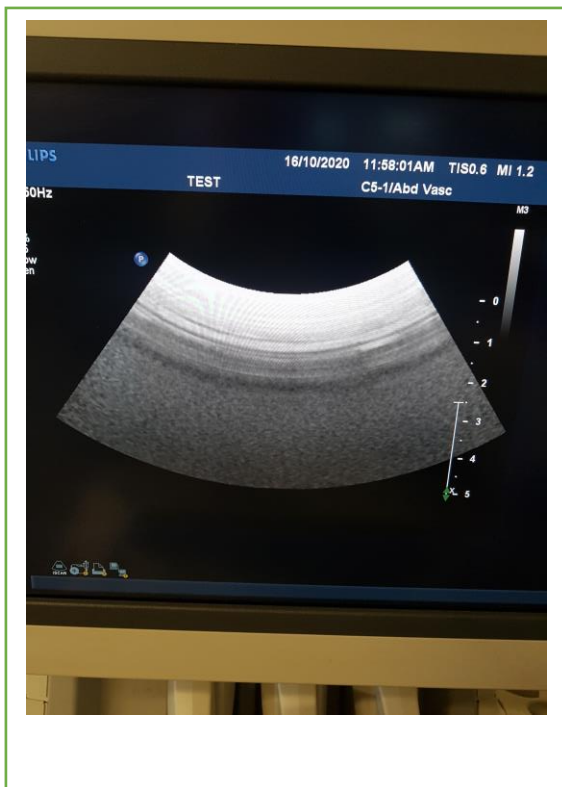


## Ultrasound Transducer Condition Report

<b>Date Tested</b> 16/10/2020	<b>Carried out By</b> – I. Rutherford
<b>Manufacturer</b> - Philips	<b>Model Number</b> – L17-5
<b>Serial Number</b> – B02YNM	
<b>Transducer Type</b> – Linear	
<b>Date of Manufacture</b> - Unknown	
<b>System used to Test</b> – Philips iU22	
<b>Cable</b> – Good	
<b>Lens</b> – Good	
<b>Discolouration</b> –Some	
<b>Overall Condition</b> – Good	

© British Medical Auctions

### Airscans –

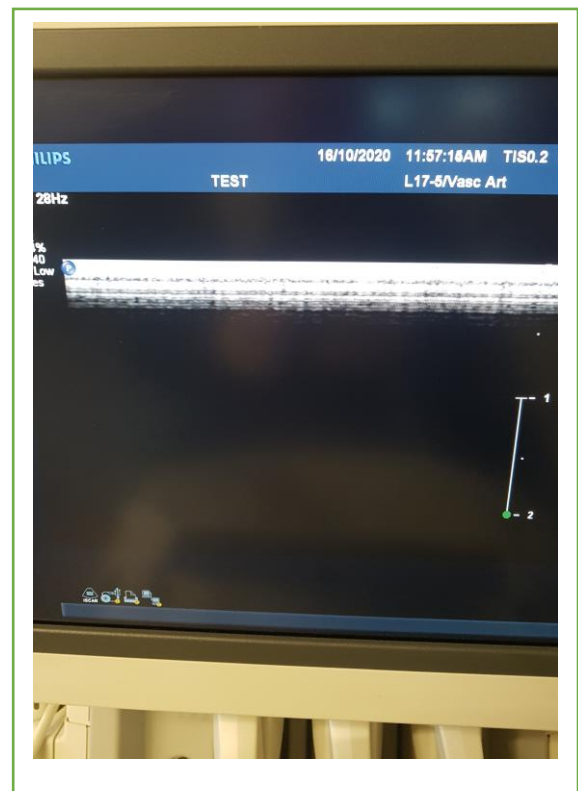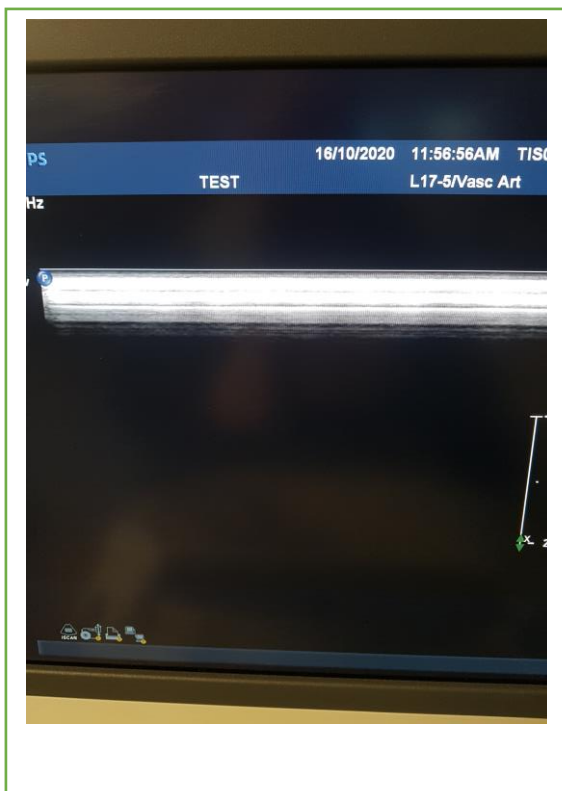

## Ultrasound Transducer Condition Report

<b>Date Tested</b> 16/10/2020	<b>Carried out By</b> – I. Rutherford
<b>Manufacturer</b> - Philips	<b>Model Number</b> – L9-3
<b>Serial Number</b> – 03H59K	
<b>Transducer Type</b> – Linear	
<b>Date of Manufacture</b> - Unknown	
<b>System used to Test</b> – Philips iU22	
<b>Cable</b> – Good	
<b>Lens</b> – Good	
<b>Discolouration</b> –Some	
<b>Overall Condition</b> – Good	

© British Medical Auctions

### Airscans –

