
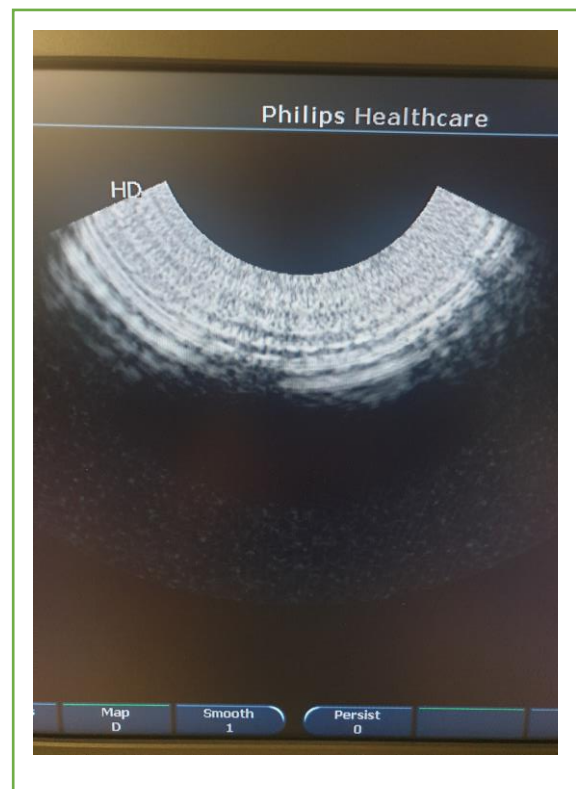


Ultrasound Transducer Condition Report

Date Tested - 20/02/2021	Carried out By - I Rutherford
Manufacturer - Philips	Model Number - C8-4v
Serial Number - 038YXM	
Transducer Type - Endocavity	
Date of Manufacture - Unknown	
System used to Test - Philips HD7 XE	
Cable - Good	
Lens - Good	
Discolouration - Slight	
Overall Condition - Good	© British Medical Auctions

Airscans -

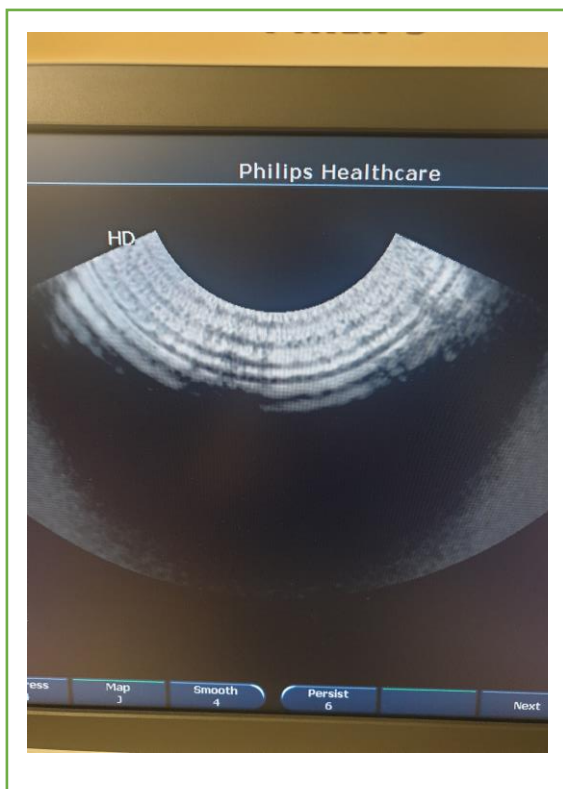

Ultrasound Transducer Condition Report

Date Tested - 20/01/2021	Carried out By – I Rutherford
Manufacturer - Philips	Model Number – C6-3
Serial Number -940909	
Transducer Type Convex	
Date of Manufacture – Unknown	
System used to Test – Philips HD7 XE	
Cable – Good	
Lens – Good	
Discolouration – Minimal	
Overall Condition - Good	

© British Medical Auctions

Airscans –

